



## Veratox Procedure for Histamine

**Note: Samples must be diluted before performing test.**


Please read kit instructions completely before beginning. Questions? Call 800/234-5333 or 517/372-9200.

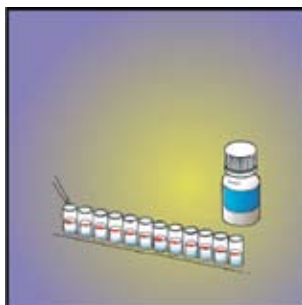

1. Add 100  $\mu$ L conjugate to each red marked mixing well.

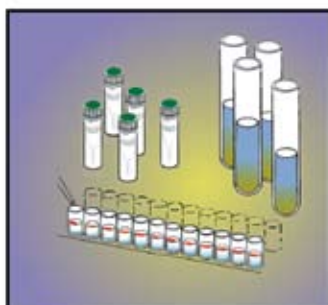

2. Add 100  $\mu$ L of controls and diluted samples to their respective wells.

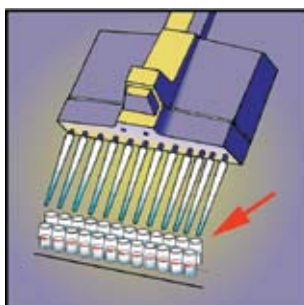

3. Mix. Transfer 100  $\mu$ L to antibody wells. Incubate for 10 minutes.




4. Dump liquid from antibody wells.




5. Wash wells thoroughly 4 times with diluted wash buffer.



6. Carefully tap out remaining liquid on absorbent paper towel.

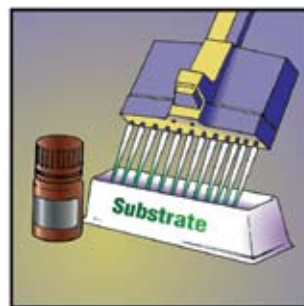

7. Transfer 100  $\mu$ L substrate from reagent boat to antibody wells using 12-channel pipettor. Incubate for 10 minutes.

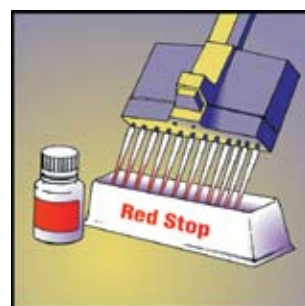

8. Transfer 100  $\mu$ L Red Stop from reagent boat to antibody wells.



9. Read results using a microwell reader with a 650 nm filter.

### Product Specifications

Lower limit of detection: 2 ppm

Range of quantitation: 2.5 ppm - 50 ppm

Controls provided: 0, 2.5, 5, 10, 20 and 50 ppm

Testing time: 20 minutes

Antibody cross-reactivity: Specific for histamine



620 Leshar Place • Lansing, MI 48912  
800/234-5333 (USA and Canada only) • 517/372-9200 • fax: 517/372-2006  
e-mail: [foodsafety@neogen.com](mailto:foodsafety@neogen.com) • [www.neogen.com](http://www.neogen.com)